

Light Measurement Report

Print date: 1/7/2026

Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS

Measurement tracking No. and Link: [n/a](#)

Operator:



Laboratory and Equipment

Laboratory Owner and Location

Goniospectrometer System and Type

Sensor Name, Calibr. Date and Serial No.

Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark

LabSpion – Type C, horizontal

LabSensor Model2 – 4/8/2025 – 1516006613

Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

Measurement Conditions

Number of C-planes and Resolution

γ (gamma)-Resolution

Test Distance

Input Power, Power and Displ. Factors

Input RMS Voltage and Current

Frequency of Input Power

Warm-up Time and Variation

12 planes – 30°

5°

10.57 m

12.5 W – PF 0.99 – DPF 0.99

121 V – 0.105 A

60 Hz

Not completed – 2.0%

Tested Light Source

Product Name

Item No. and Manufacturer

Product Description (line 1)

HP1-P-I-4'-B-835-F-BLX2835

HP1-P-I-4'-B-835-F-BLX2835 – Finelite Inc.

Main Light Measurement Results

Output – Total Lumen (Up% / Down%)

Efficiency

Peak Intensity and Beam Angle

Correlated Color Temperature, Target/Measured

Color Rendering Index

Color Rendering TM30-18

Color Shift, CIE duv and MacAdam Steps

Flicker

1520 lm – 0.65% / 99.35%

122 lm/W

600 cd – 100.2°



CCT = 3487 K / 3487 K

CRI 83.0

R_f 84.2 – R_g 97.6

Duv 0.0006 – SDCM n/a

SVM n/a – PstLM n/a

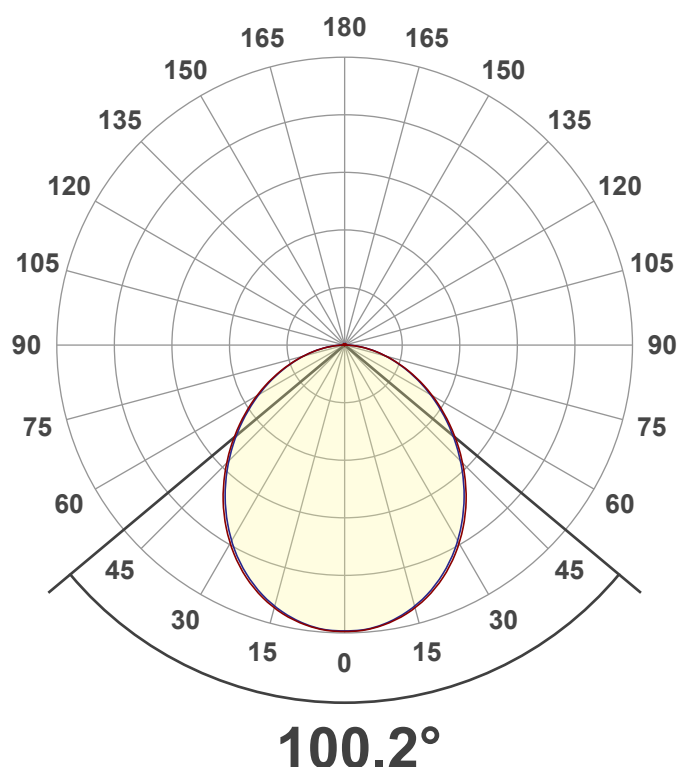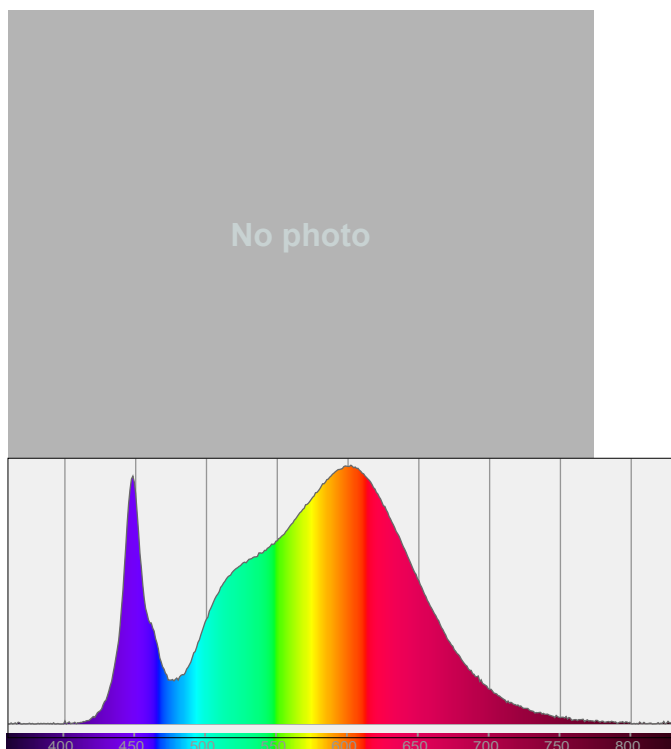

Light Measurement Report

Print date: 1/7/2026

Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS


Measurement tracking No. and Link: [n/a](#)

Operator:



Luminous Intensity diagram

Unit: 0-100% of peak intensity

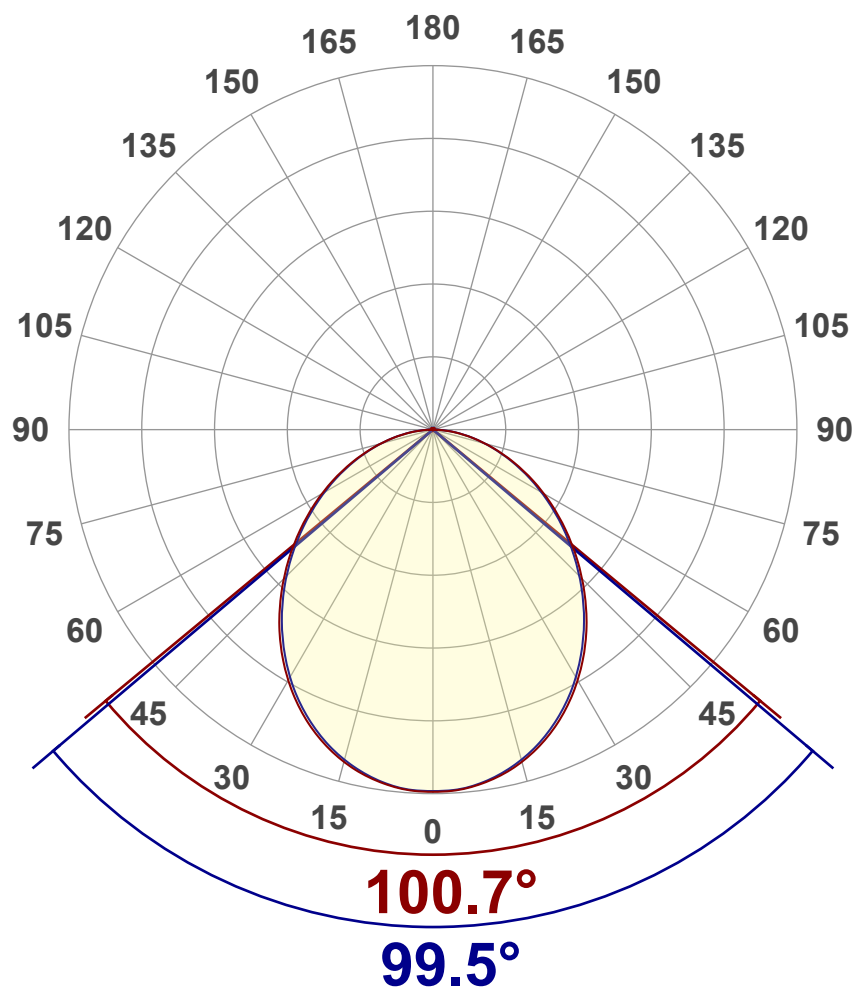

Main Values

Output (total Lumen)	1520 lm
Lumen Up% / Down%	0.65% / 99.35%
Peak Intensity	600 cd
Beam Angle (50%)	100.2°
Beam Angle (90%)	99.5°
Beam Angle (10%)	100.7°

Cut-off Angle

Average 2,5%	174.8°
--------------	--------

Field Angle

Average 10%	158.8°
-------------	--------


Intensity Ratio

In 120° cone	80.2%
In 90° cone	56.7%

C000-C180

C090-C270

Linear distribution diagram - Intensity (candela) vs γ-angle

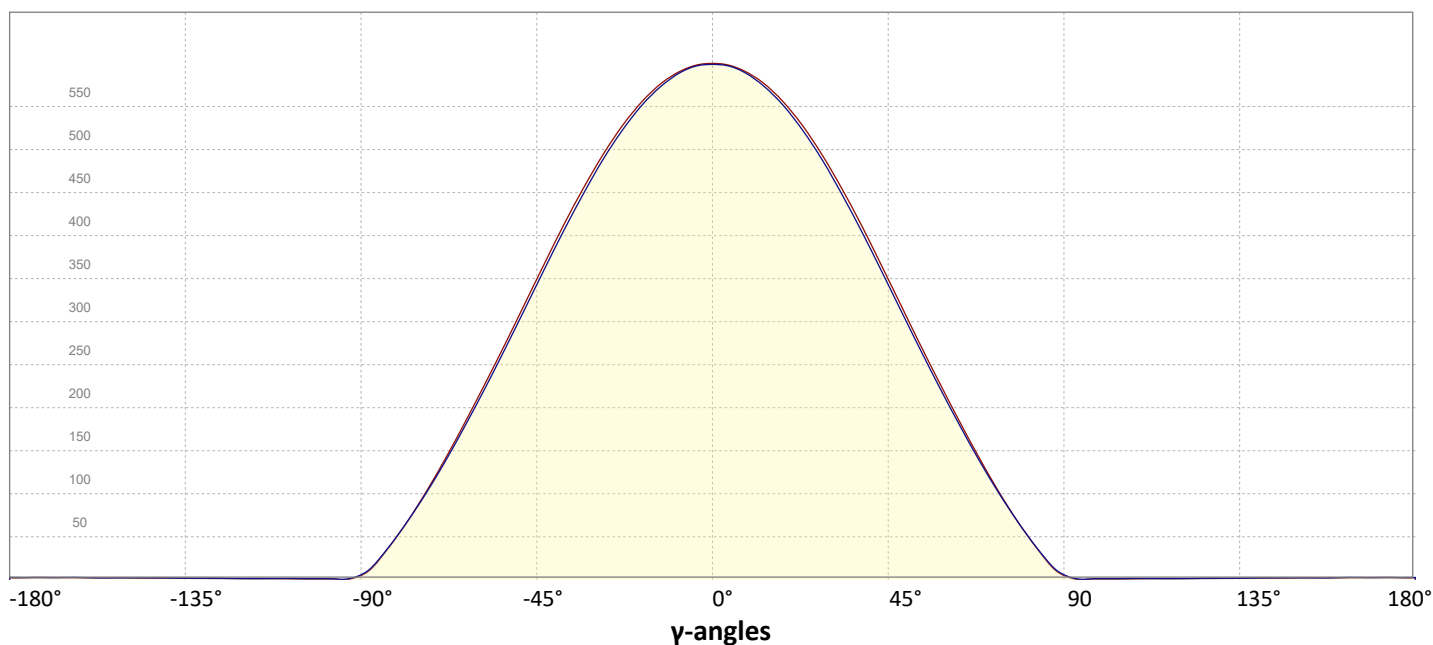


Light Measurement Report


Print date: 1/7/2026
Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS
Measurement tracking No. and Link: [n/a](#)
Operator:



Iso-intensity Diagram (Iso-candela)

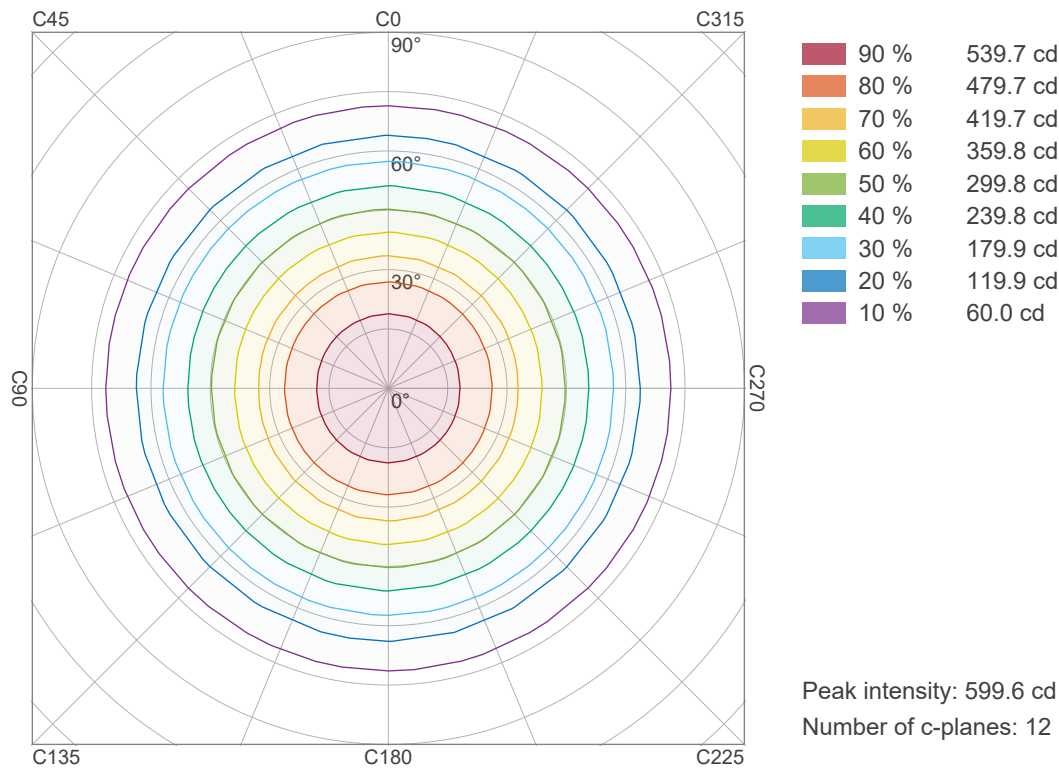

Iso-illuminance Diagram (Iso-lux)

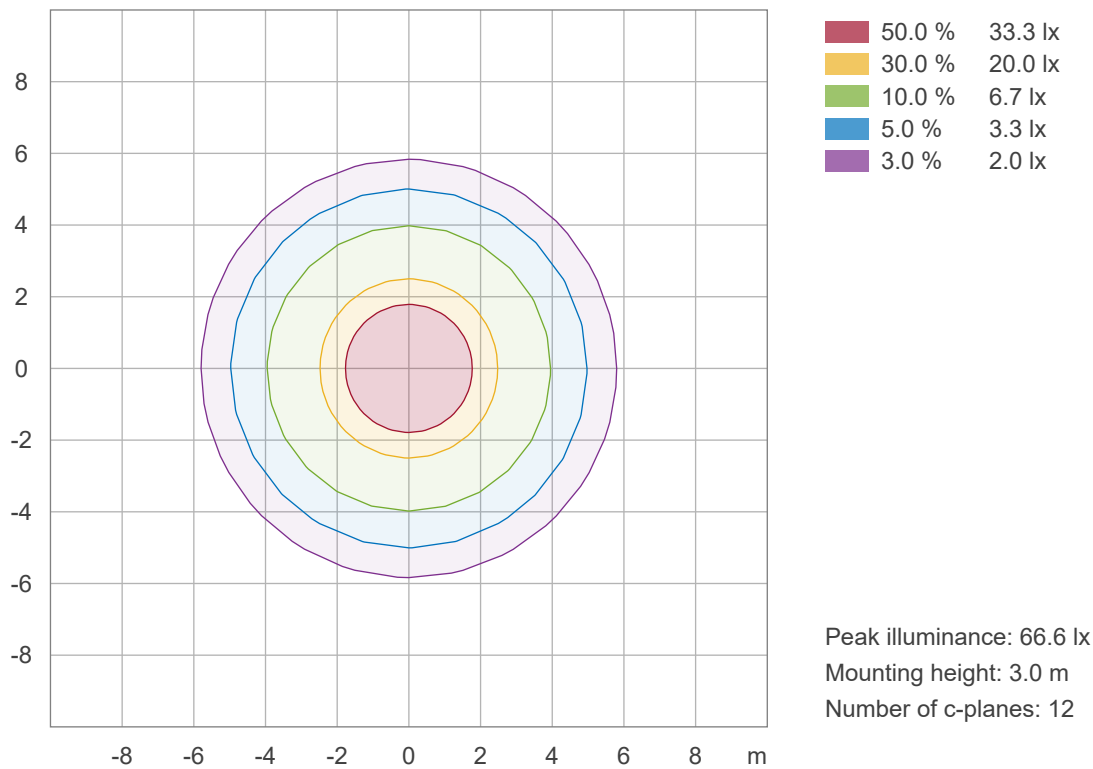

Light Measurement Report

Print date: 1/7/2026

Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS

Measurement tracking No. and Link: [n/a](#)

Operator:




Color details


Correlated Color Temperature, Target CCT = 3487 K
Correlated Color Temperature, Measured CCT = 3487 K
Color Rendering Index CRI 83.0
Color Rendering Index, R9 (red component) R9 = 9.5
Color Rendering TM30-18 R_f 84.2 – R_g 97.6
Color Quality Scale CQS = 83.0

MacAdam Steps
Color coordinates CIE 1931 (x;y) = (0.407;0.393)
Color coordinate CIEs 1960 (u;v) = (0.236;0.342)
Color deviation from BBL Duv = 0.0006
Color coordinate CIEs 1976 (CIELUV) (u';v') = (0.236;0.512)


CIE 1931

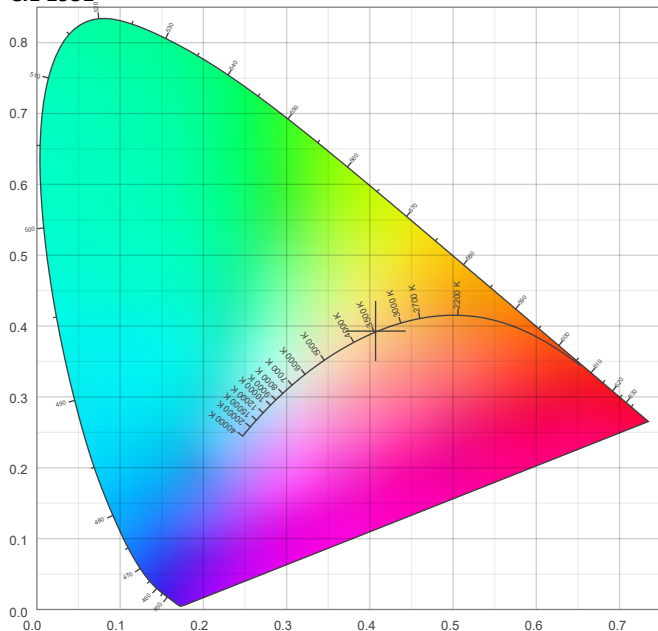

CIE 1931 – zoomed on Planckian locus

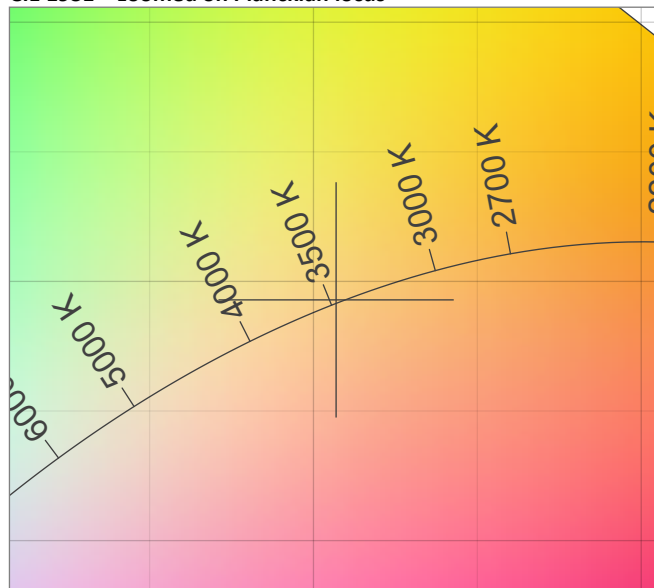


Color Rendering Index per reference color (CIE 1995)

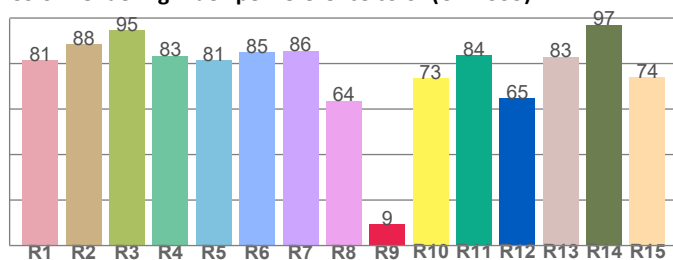


CRI R values, only R1-R8 are used to calculate final CRI value

R1	R2	R3	R4	R5	R6	R7	R8	R9	R10	R11	R12	R13	R14	R15
81.5	88.4	94.7	83.4	81.5	85.0	85.6	63.7	9.5	73.5	83.6	64.8	83.0	97.1	73.9

Spectral power distribution (SPD) / W/nm – 0-100%

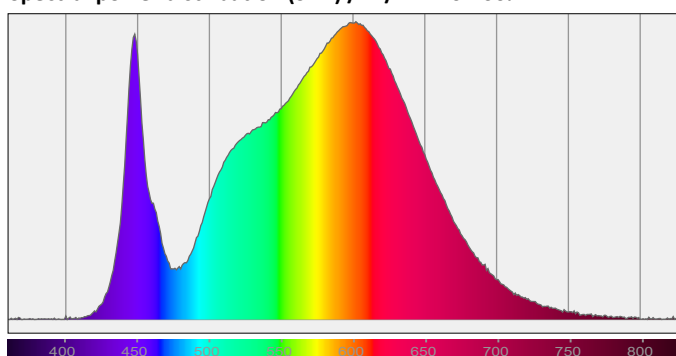


TM30-18 R_f-values per hue bin

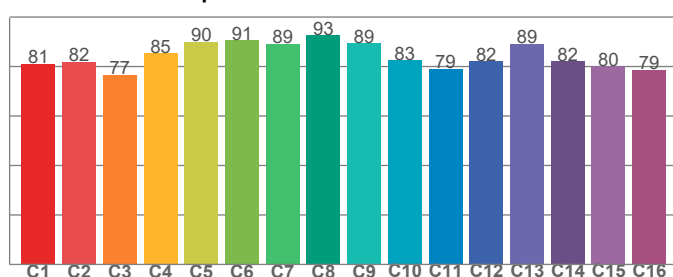

TM30 C values, 16 binned values out of total of 99 C values

C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
81.1	82.0	76.6	85.4	90.0	90.6	89.2	92.7	89.3	82.5	79.1	82.2	89.2	82.2	80.2	78.7

Color Quality Scale by reference color

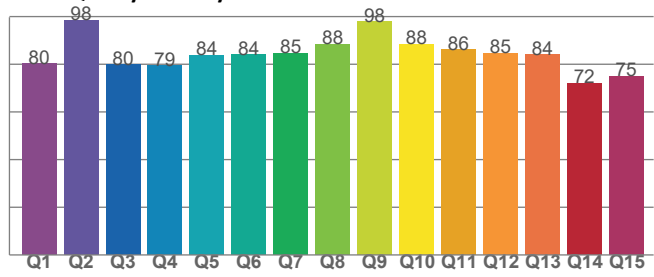

CQS Q values

Q1	Q2	Q3	Q4	Q5	Q6	Q7	Q8	Q9	Q10	Q11	Q12	Q13	Q14	Q15
80.2	98.5	79.8	79.4	83.8	84.0	84.6	88.4	97.9	88.3	86.1	84.5	84.0	72.1	74.9

Light Measurement Report

Print date: 1/7/2026


Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS

Measurement tracking No. and Link: [n/a](#)

Operator:



Beam Details

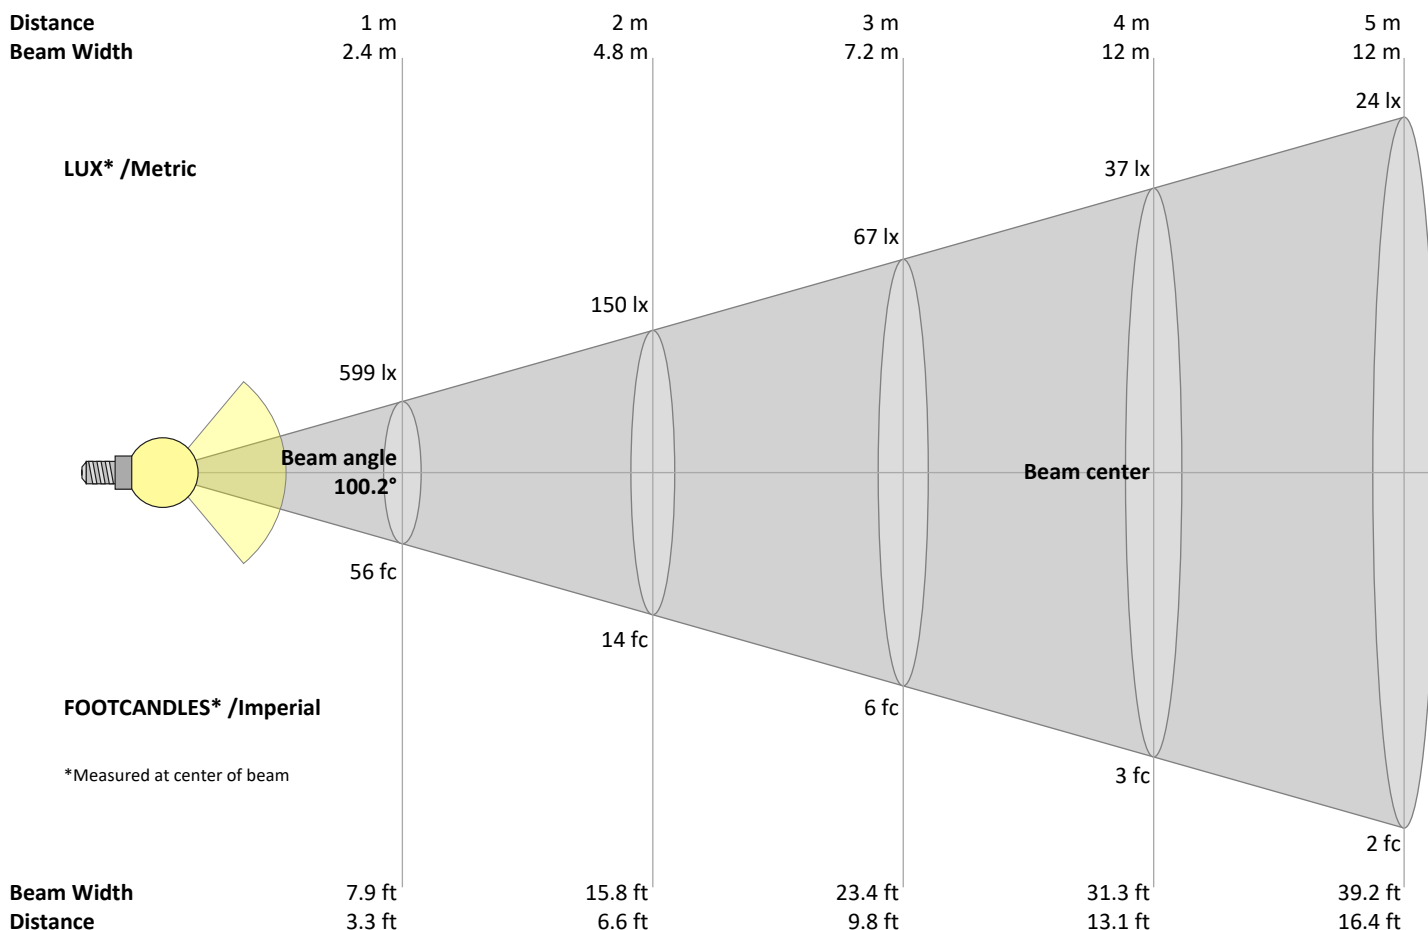

Beam intensities from 1 – 20 m

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	m
3.3	6.6	9.8	13.1	16.4	19.7	23	26.2	29.5	32.8	36.1	39.4	42.7	45.9	49.2	52.5	55.8	59.1	62.3	65.6	ft
599	150	67	37	24	17	12	9	7	6	5	4	4	3	3	2	2	2	2	1	lux
55.6	13.9	6.2	3.5	2.2	1.5	1.1	0.9	0.7	0.6	0.5	0.4	0.3	0.3	0.2	0.2	0.2	0.2	0.2	0.1	fc

Intensities in 0° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
599	596	586	569	545	515	479	439	395	349	303	257	212	169	128	90	56	26	7	1	cd
100%	100%	98%	95%	91%	86%	80%	73%	66%	58%	51%	43%	35%	28%	21%	15%	9%	4%	1%	0%	of 0°val

Intensities in 90° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
599	595	584	565	540	509	473	432	388	343	297	252	208	166	126	89	56	27	7	1	cd
100%	99%	98%	94%	90%	85%	79%	72%	65%	57%	50%	42%	35%	28%	21%	15%	9%	5%	1%	0%	of 0°val

Intensities in 180° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
599	596	586	569	545	515	479	439	395	349	303	257	212	169	128	90	56	26	7	1	cd
100%	100%	98%	95%	91%	86%	80%	73%	66%	58%	51%	43%	35%	28%	21%	15%	9%	4%	1%	0%	of 0°val

Intensities in 270° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
599	595	584	565	540	509	473	432	388	343	297	252	208	166	126	89	56	27	7	1	cd
100%	99%	98%	94%	90%	85%	79%	72%	65%	57%	50%	42%	35%	28%	21%	15%	9%	5%	1%	0%	of 0°val

Light Measurement Report


Print date: 1/7/2026
Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS
Measurement tracking No. and Link: [n/a](#)
Operator:



Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

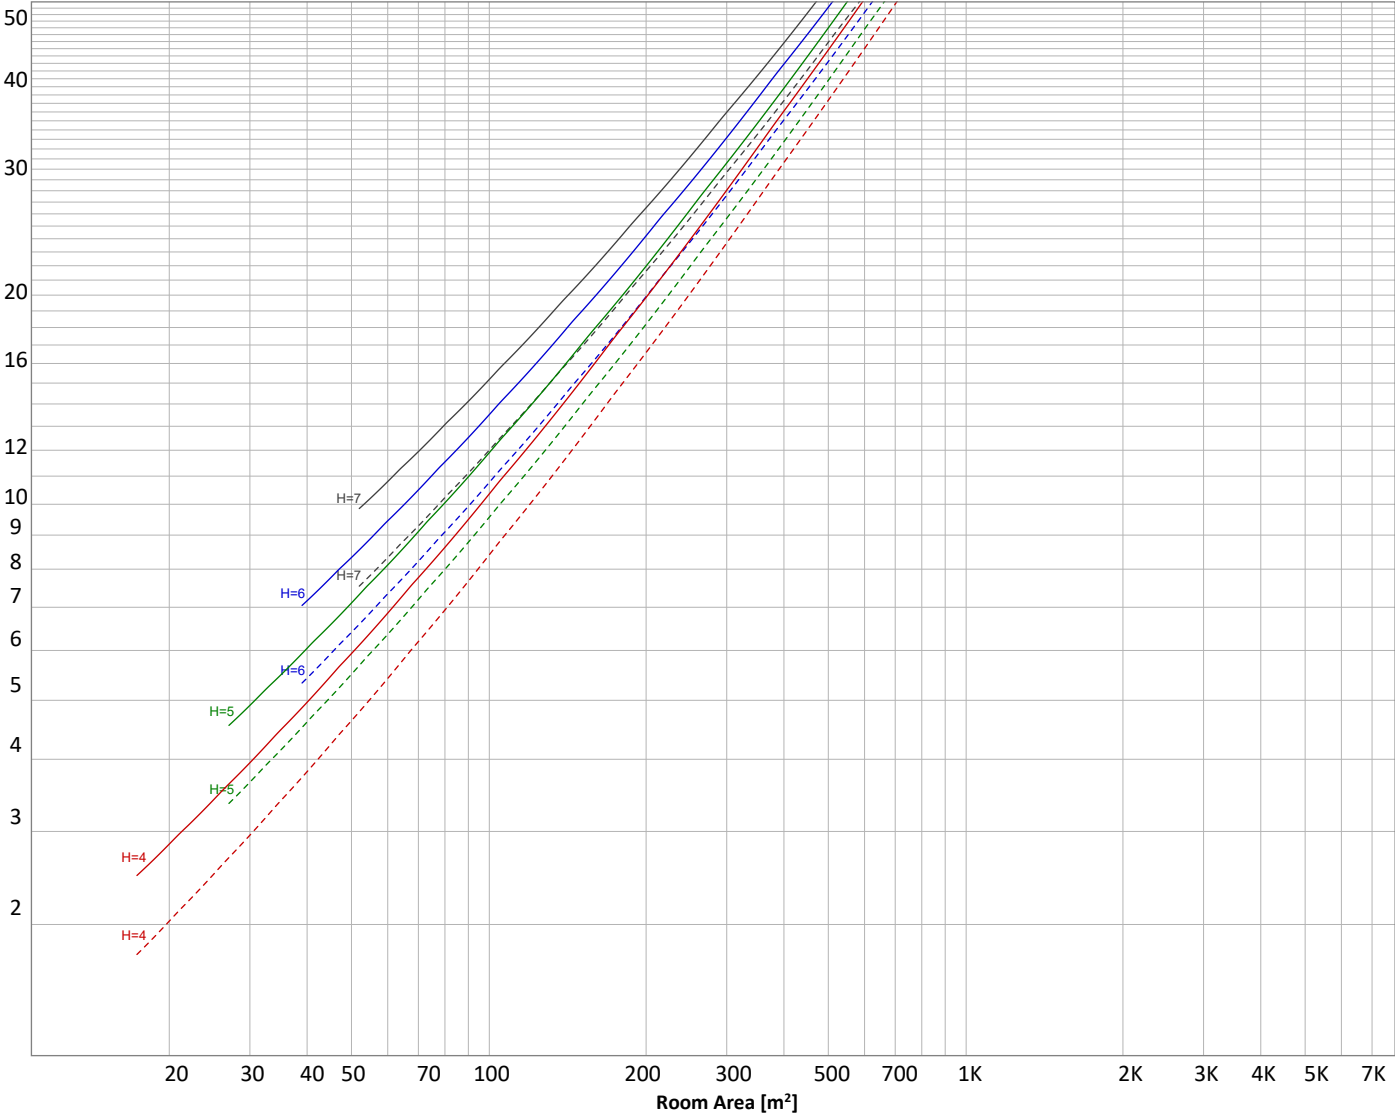

Conditions

H = Room height	Flux = 1520 lm	p(%)		
H _{down} = Lamp distance from ceiling =	0.00 m	Line type	Ceiling reflectance	Wall reflectance
H _{work} = Work area height from floor =	0.00 m	-----	70	50
E _{work} = Average lux on work area =	100 lx	-----	50	30
				Floor reflectance
				20

Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
56.6 lm	160 lm	236 lm	272 lm	267 lm	228 lm	166 lm	94.8 lm	29.9 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
1.74 lm	1.11 lm	1.26 lm	1.29 lm	1.29 lm	1.30 lm	1.02 lm	0.685 lm	0.235 lm

Light Measurement Report

Print date: 1/7/2026

Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS

Measurement tracking No. and Link: [n/a](#)

Operator:



Outdoor Light Planning

Lumen per Zone

Zone (γ)	Lumen	% Total
0-10°	57 lm	3.7%
10-20°	160 lm	10.5%
20-30°	236 lm	15.5%
30-40°	272 lm	17.9%
40-50°	267 lm	17.6%
50-60°	228 lm	15.0%
60-70°	166 lm	10.9%
70-80°	95 lm	6.2%
80-90°	30 lm	2.0%
90-100°	2 lm	0.1%
100-110°	1 lm	0.1%
110-120°	1 lm	0.1%
120-130°	1 lm	0.1%
130-140°	1 lm	0.1%
140-150°	1 lm	0.1%
150-160°	1 lm	0.1%
160-170°	1 lm	0.0%
170-180°	0 lm	0.0%
Total	1520 lm	100.0%

Intensity peaks

Max intensity	600 cd
Intensity, 90°	7 cd
Intensity, 0°	599 cd

Zonal Lumen summary

Zone (γ)	Lumen	% Total
0-30°	452 lm	29.8%
0-40°	725 lm	47.7%
0-60°	1220 lm	80.2%
60-90°	290 lm	19.1%
70-100°	126 lm	8.3%
90-120°	4 lm	0.3%
0-90°	1510 lm	99.3%
90-180°	10 lm	0.7%
0-180°	1520 lm	100.0%

BUG rating

	Lumen	% Total
Forward light		
Low(0-30°)	226 lm	14.9%
Medium(30-60°)	383 lm	25.2%
High(60-80°)	130 lm	8.6%
Very high(80-90°)	15 lm	1.0%
Back light		
Low(0-30°)	226 lm	14.9%
Medium(30-60°)	383 lm	25.2%
High(60-80°)	130 lm	8.6%
Very high(80-90°)	15 lm	1.0%


Uplight

Low(90-100°)	2 lm	0.1%
High(100-180°)	8 lm	0.5%

IESNA TM-15-07

Luminaire Classification System For Outdoor Luminaires

BUG rating B1 U1 G1

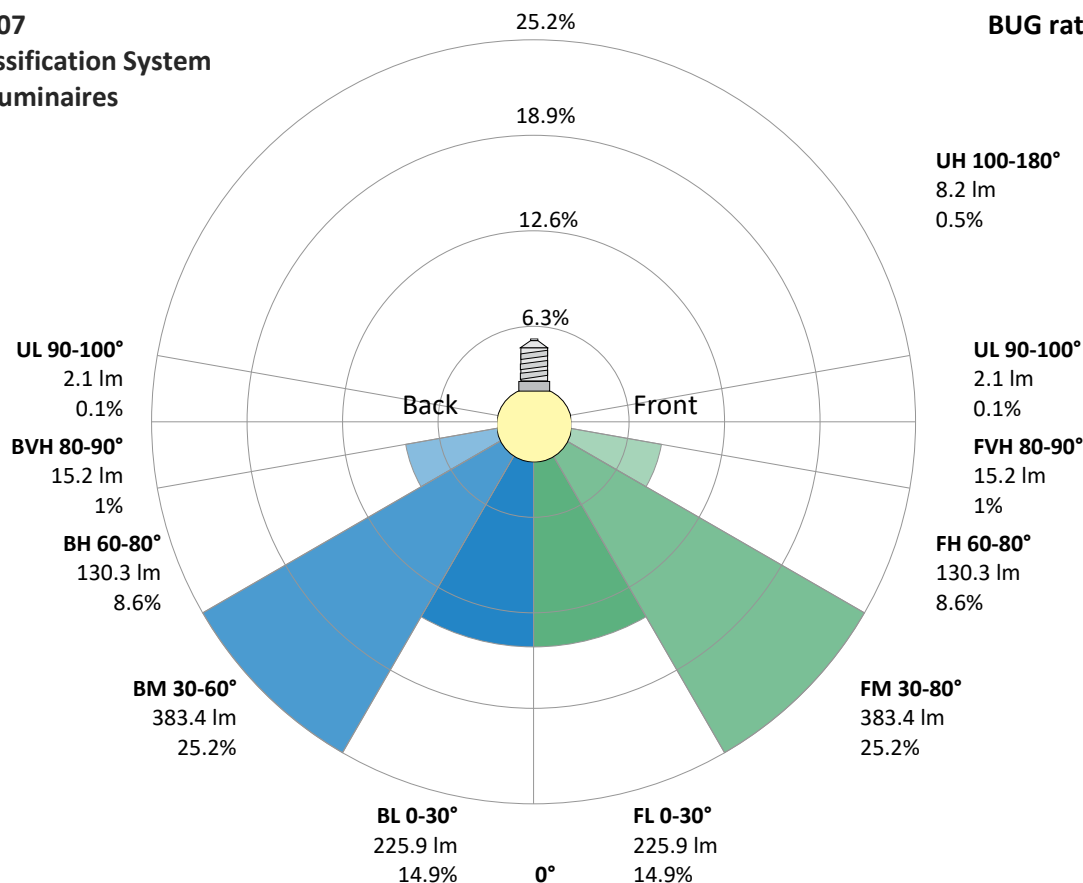

Light Measurement Report

Print date: 1/7/2026
Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS
Measurement tracking No. and Link: [n/a](#)
Operator:




Power Details


Input Power

Power feed to light source	12.5 W
Frequency of input power	60 Hz
RMS Input voltage feed, V_{RMS}	121 V
RMS Input current feed, I_{RMS}	0.105 A
Volt-Ampere or apparent power = $V_{RMS} \cdot I_{RMS}$	12.67 VA
Displacement factor of AC power feed	0.99
Power factor of AC current feed	0.99
Total harmonic distortion of the current	6.65%
Total harmonic distortion of the voltage	2.05%

Input Power Curve

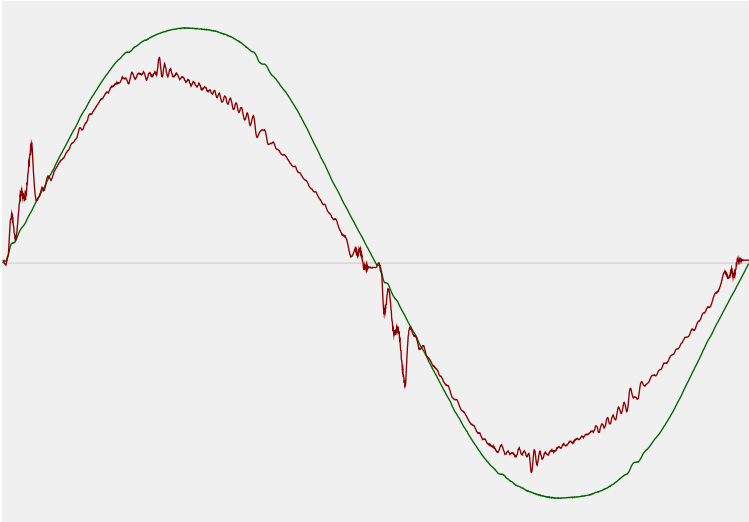

Efficiency

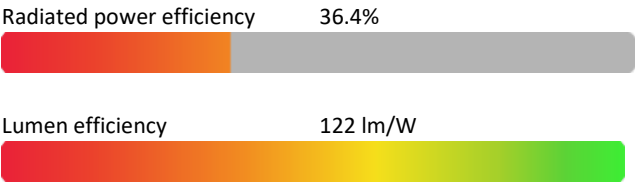

Stabilization Details

Warmup Conditions

Stable period	15 min
Stable change max	2.0%
Minimum time	15 min

Color Temperature Change

CCT start	3486 K
CCT shift	+1 K
CCT end	3487 K


Warmup Result

Total warmup time	Not completed
Warmup variation	-0.6%

Output Change

Output start	1523 lm
Output change	-3 lm
Output end	1520 lm

Stabilization Curve

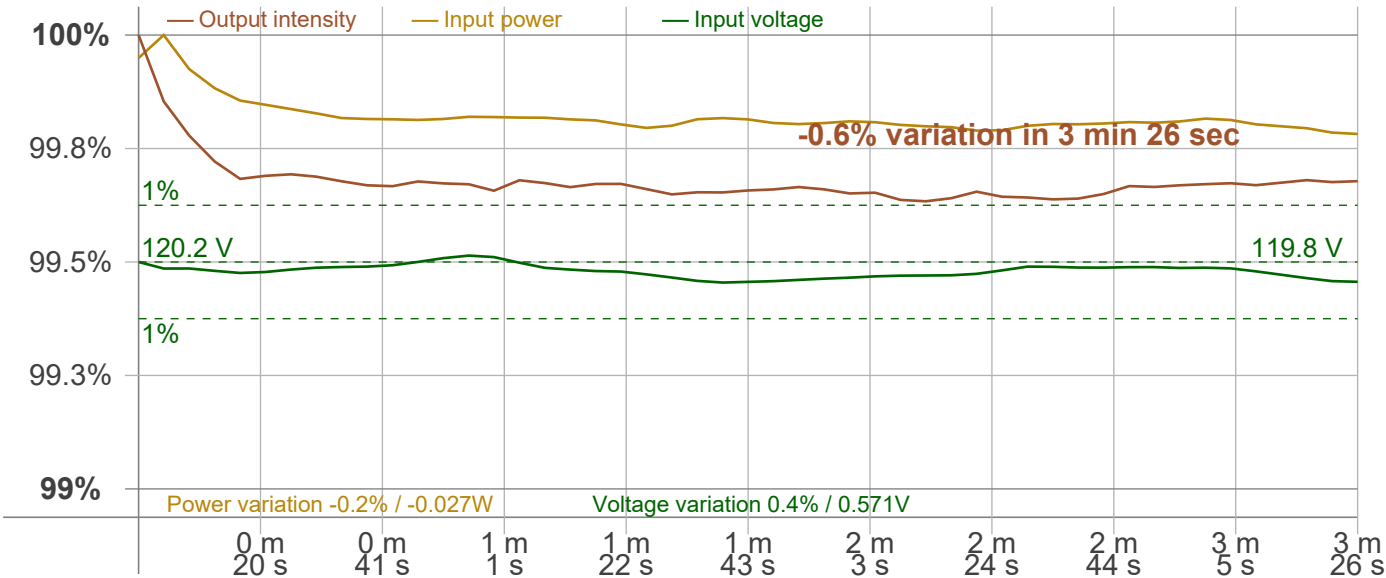

Light Measurement Report


Print date: 1/7/2026
Measurement date and time: 1/7/2026 5:10:44 PM – Measurement no. VFR-260107-0782-MS
Measurement tracking No. and Link: [n/a](#)
Operator:




Flicker /TLA details

Flicker Meter Type	Viso Systems LabFlicker	Measurement time	
Frequency of input power	60 Hz	PstLM	180 sec
Flicker/TLA sample rate	n/a samples/s	All other indices	1,2 sec
Flicker indices according to Illuminating Engineering Society (IES)		Flicker indices according to California Energy Commission (CEC) 2016b	
Flicker frequency	n/a Hz	JA8/10 40 Hz	n/a %
Percent Flicker	n/a %	JA8/10 90 Hz	n/a %
Flicker index	n/a	JA8/10 200 Hz	n/a %
		JA8/10 400 Hz	n/a %
		JA8/10 1000 Hz	n/a %
TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)		Flicker indices according to Lighting Research Center (2015)	
PstLM value (F < 80 Hz)	n/a	Perception metric, Assist Mp	n/a
SVM value (80 < F < 2000 Hz)	n/a		

Flicker frame (frame of one flicker period in time domain)

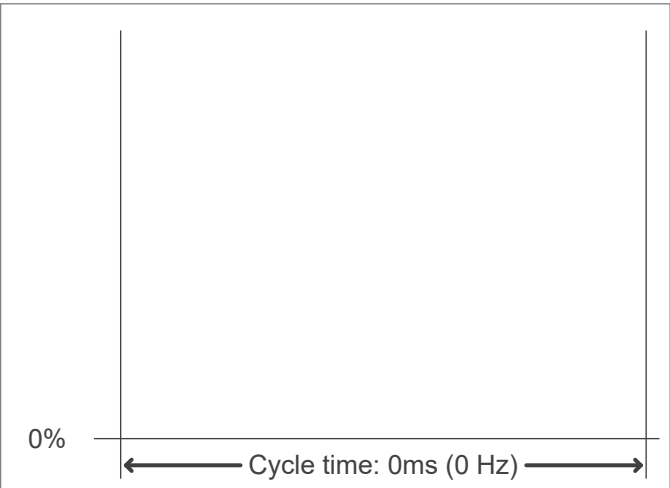

Flicker FFT (flicker curve in frequency domain)

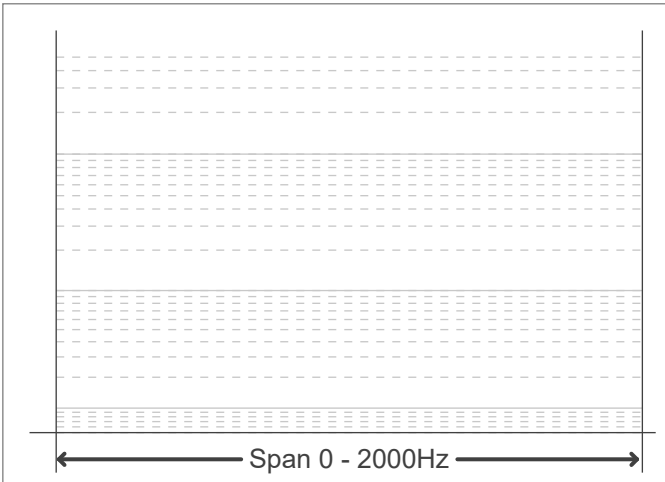

IEEE 1789 Frequency/modulation plot

